


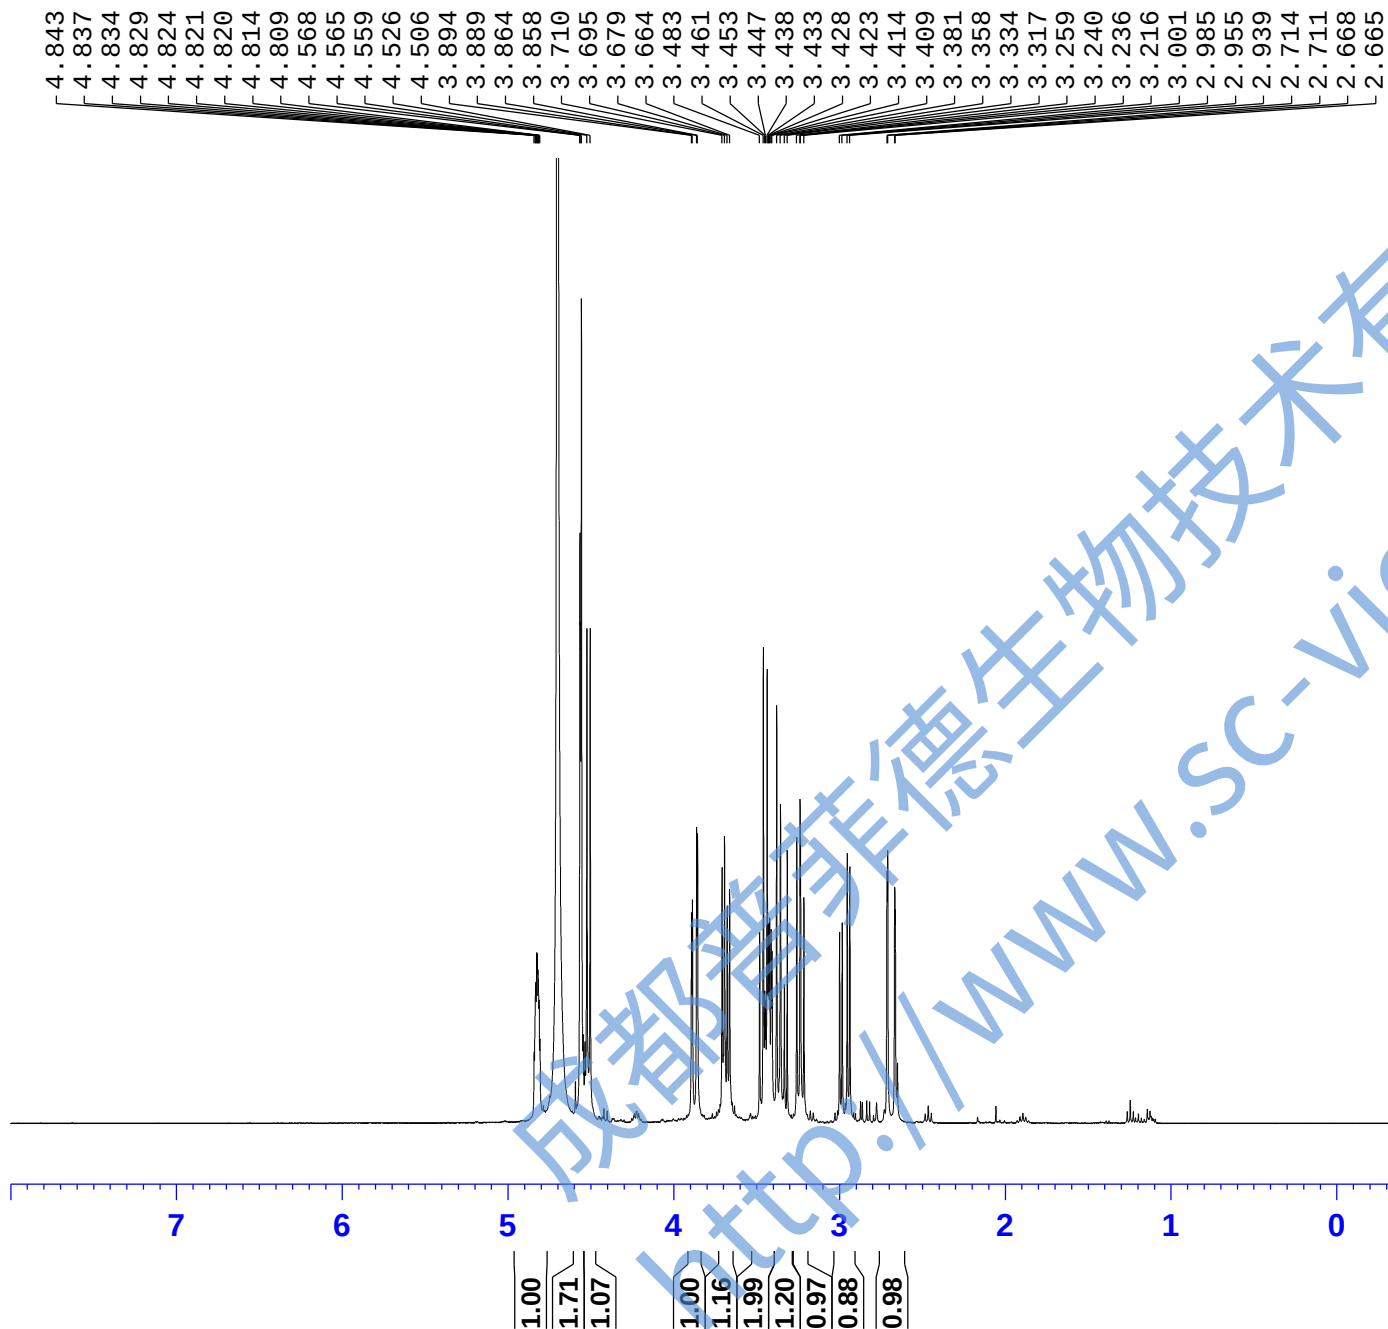

Current Data Parameters
 NAME JXLG-1H NMR D2O
 EXPNO 1
 PROCNO 1

F2 - Acquisition Parameters
 Date 20161019
 Time 10.11
 INSTRUM spect
 PROBHD 5 mm PABBO BB/
 PULPROG zg30
 TD 65536
 SOLVENT D2O
 NS 32
 DS 2
 SWH 8012.820 Hz
 FIDRES 0.122266 Hz
 AQ 4.0894465 sec
 RG 57.2
 DW 62.400 usec
 DE 6.50 usec
 TE 301.1 K
 D1 2.00000000 sec
 TD0 1

===== CHANNEL f1 =====
 SF01 400.1324710 MHz
 NUC1 1H
 P1 14.79 usec
 PLW1 11.50800037 W

F2 - Processing parameters
 SI 262144
 SF 400.1300000 MHz
 WDW EM
 SSB 0
 LB 0.30 Hz
 GB 0
 PC 1.00
 SR 0 Hz

4.843
4.837
4.834
4.829
4.824
4.821
4.820
4.814
4.809

4.568
4.565
4.559
4.526
4.506


BRUKER

Current Data Parameters
NAME JXLG-1H NMR D2O
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters
Date 20161019
Time 10.11
INSTRUM spect
PROBHD 5 mm PABBO BB/
PULPROG zg30
TD 65536
SOLVENT D2O
NS 32
DS 2
SWH 8012.820 Hz
FIDRES 0.122266 Hz
AQ 4.0894465 sec
RG 57.2
DW 62.400 usec
DE 6.50 usec
TE 301.1 K
D1 2.00000000 sec
TD0 1

===== CHANNEL f1 =====
SF01 400.1324710 MHz
NUC1 1H
P1 14.79 usec
PLW1 11.50800037 W

F2 - Processing parameters
SI 262144
SF 400.1300000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00
SR 0 Hz

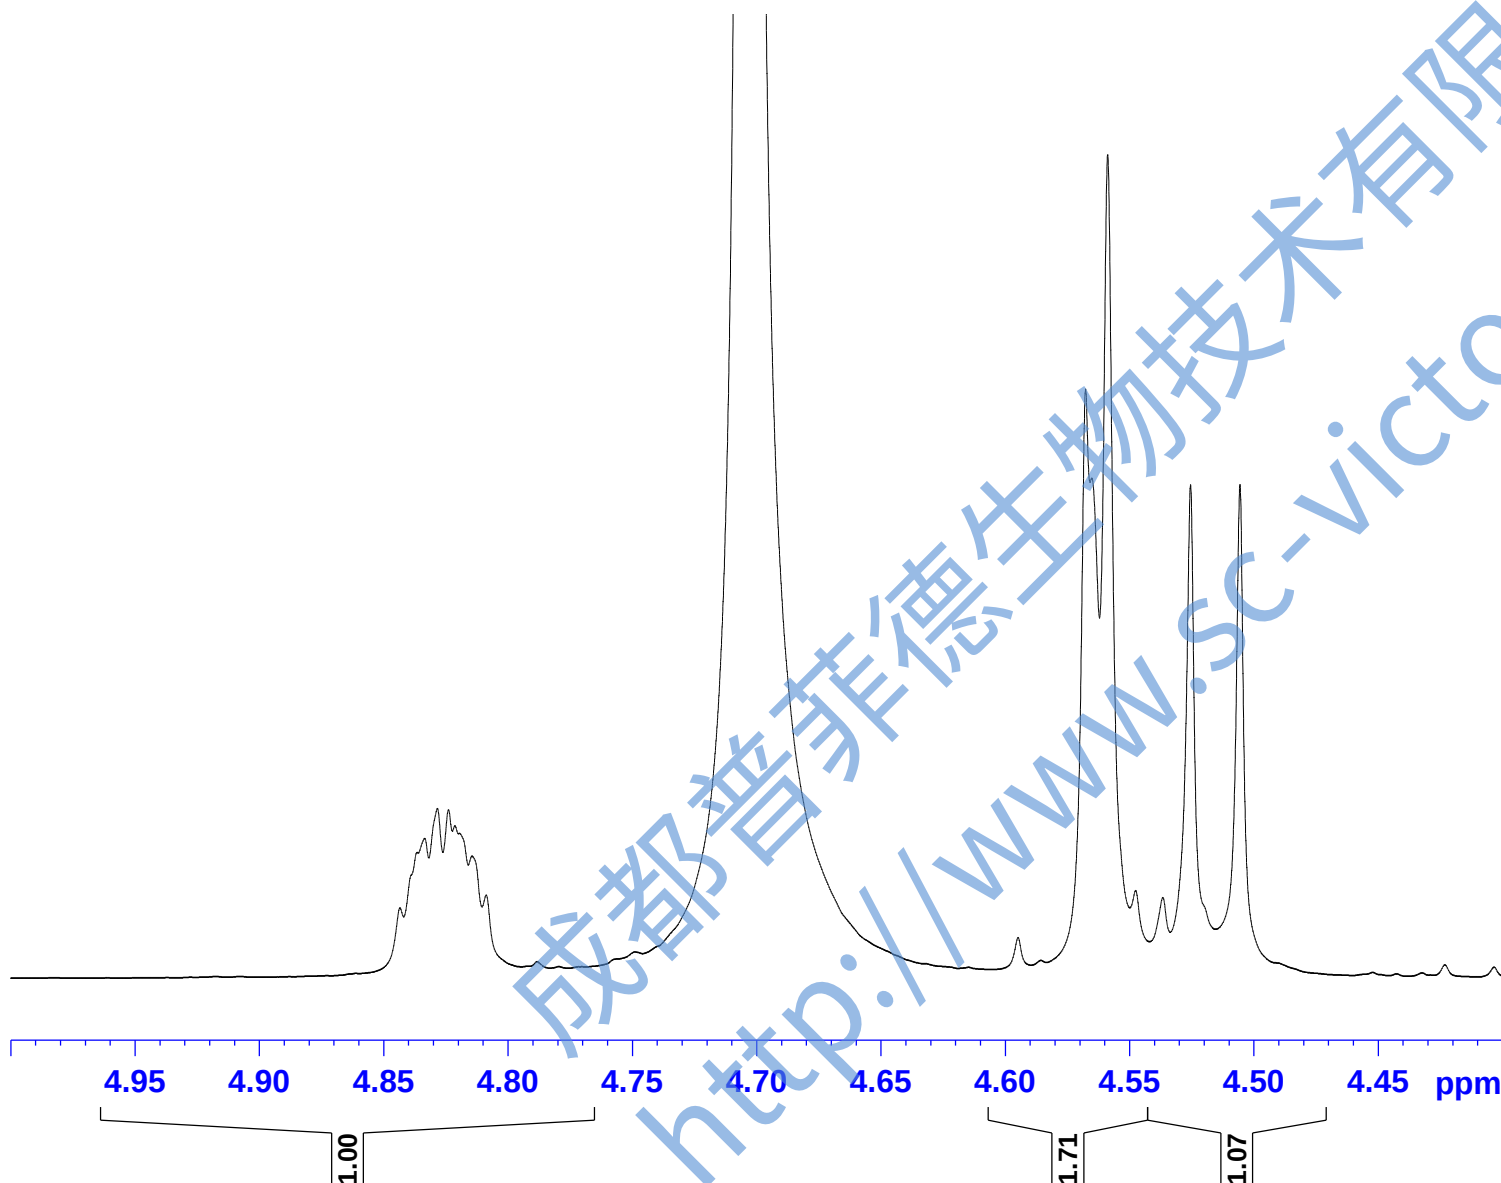

3.894
3.889

3.864
3.858

3.710

3.695

3.679

3.664




Current Data Parameters
NAME JXLG-1H NMR D2O
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20161019
Time_ 10.11
INSTRUM spect
PROBHD 5 mm PABBO BB/
PULPROG zg30
TD 65536
SOLVENT D2O
NS 32
DS 2
SWH 8012.820 Hz
FIDRES 0.122266 Hz
AQ 4.0894465 sec
RG 57.2
DW 62.400 usec
DE 6.50 usec
TE 301.1 K
D1 2.00000000 sec
TD0 1

===== CHANNEL f1 =====
SF01 400.1324710 MHz
NUC1 1H
P1 14.79 usec
PLW1 11.50800037 W

F2 - Processing parameters
SI 262144
SF 400.1300000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00
SR 0 Hz

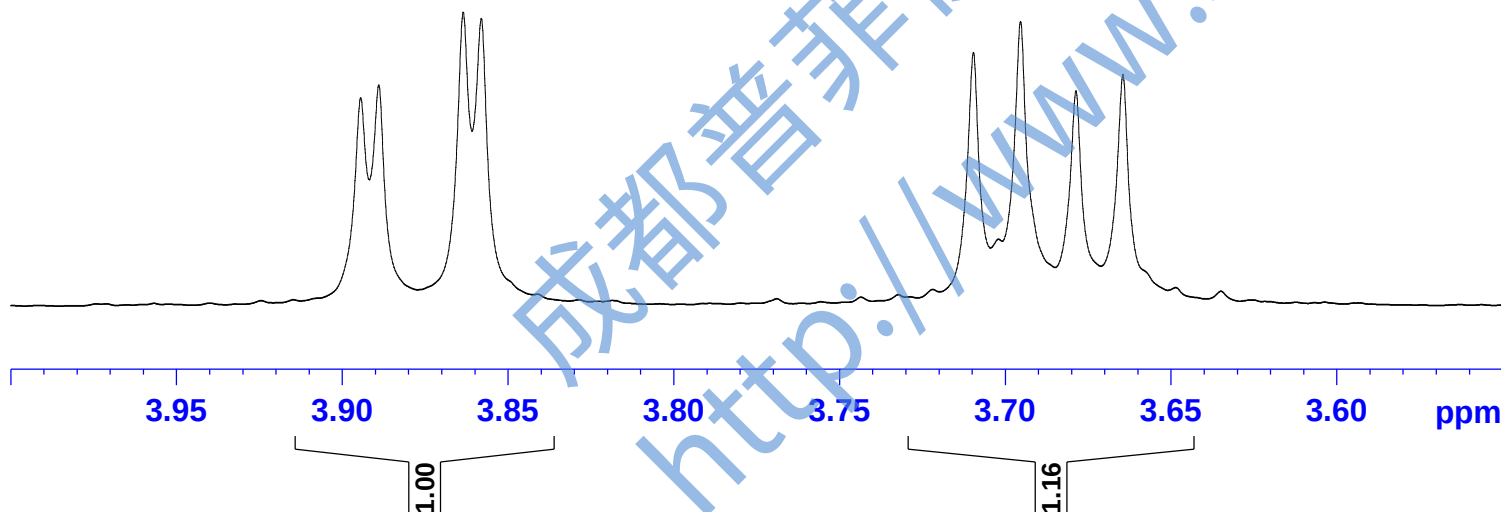

3.483
3.461
3.453
3.447
3.438
3.433
3.428
3.423
3.414
3.409
3.381
3.358
3.334
3.317
3.259
3.240
3.236
3.216




Current Data Parameters
NAME JXLG-1H NMR D2O
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters
Date 20161019
Time 10.11
INSTRUM spect
PROBHD 5 mm PABBO BB/
PULPROG zg30
TD 65536
SOLVENT D2O
NS 32
DS 2
SWH 8012.820 Hz
FIDRES 0.122266 Hz
AQ 4.0894465 sec
RG 57.2
DW 62.400 usec
DE 6.50 usec
TE 301.1 K
D1 2.00000000 sec
TD0 1

===== CHANNEL f1 =====
SF01 400.1324710 MHz
NUC1 1H
P1 14.79 usec
PLW1 11.50800037 W

F2 - Processing parameters
SI 262144
SF 400.1300000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00
SR 0 Hz

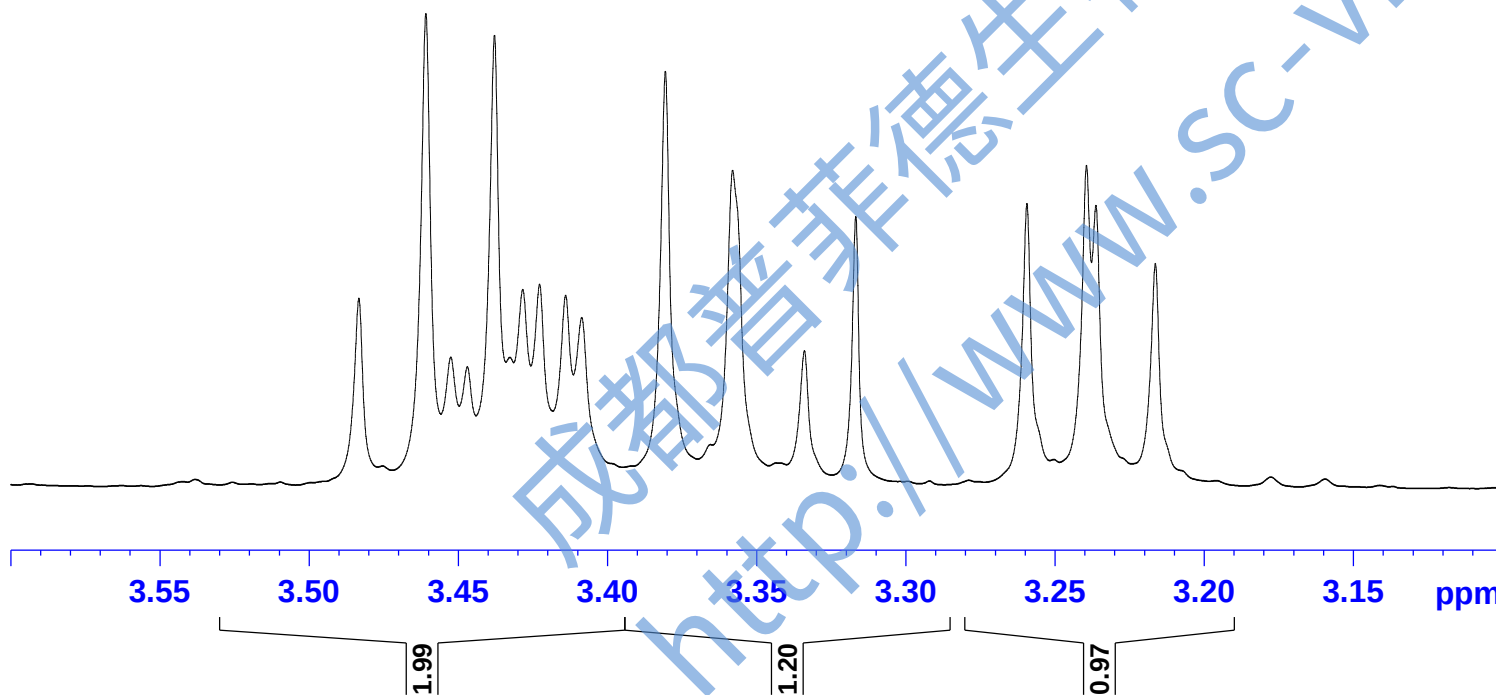

— 3.001
— 2.985

— 2.955
— 2.939

— 2.714
— 2.711

— 2.668
— 2.665




Current Data Parameters
NAME JXLG-1H NMR D2O
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters
Date 20161019
Time 10.11
INSTRUM spect
PROBHD 5 mm PABBO BB/
PULPROG zg30
TD 65536
SOLVENT D2O
NS 32
DS 2
SWH 8012.820 Hz
FIDRES 0.122266 Hz
AQ 4.0894465 sec
RG 57.2
DW 62.400 usec
DE 6.50 usec
TE 301.1 K
D1 2.00000000 sec
TD0 1

===== CHANNEL f1 =====
SF01 400.1324710 MHz
NUC1 1H
P1 14.79 usec
PLW1 11.50800037 W

F2 - Processing parameters
SI 262144
SF 400.1300000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00
SR 0 Hz

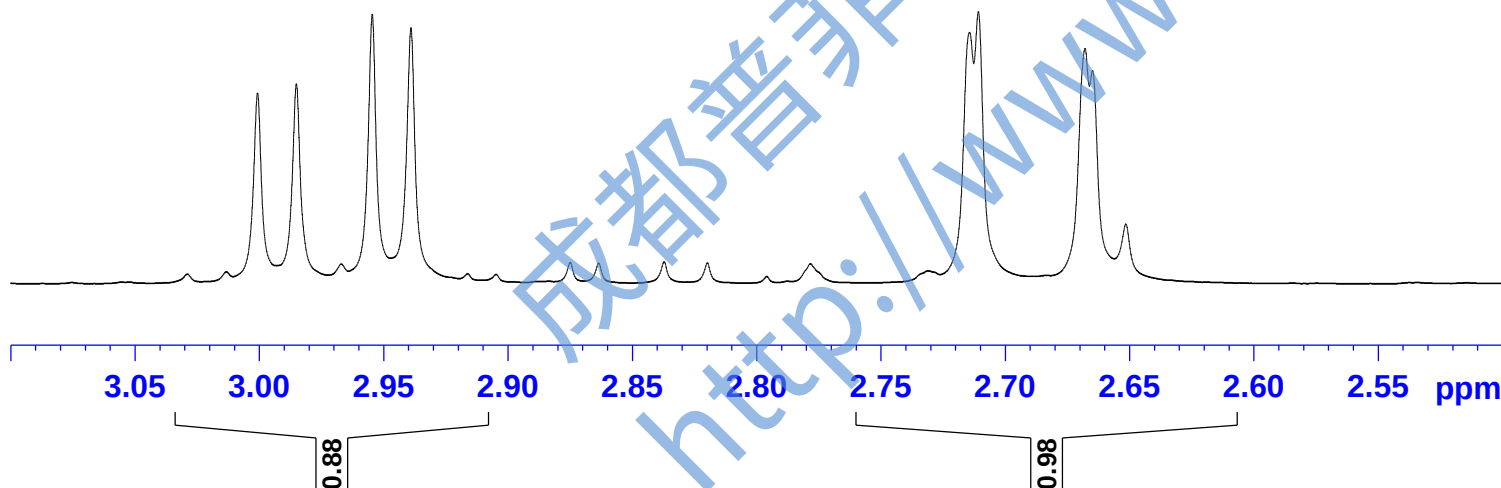

—179.69

—101.36

76.06
75.59
75.34
75.33
72.91
69.54
60.67

—35.30




Current Data Parameters
NAME JXLG-13C NMR D20
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20161019
Time 10.16
INSTRUM spect
PROBHD 5 mm PABBO BB/
PULPROG zgig30
TD 65536
SOLVENT D2O
NS 366
DS 4
SWH 24038.461 Hz
FIDRES 0.366798 Hz
AQ 1.3631488 sec
RG 202.5
DW 20.800 usec
DE 6.50 usec
TE 301.2 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1

===== CHANNEL f1 =====
SF01 100.6228298 MHz
NUC1 13C
P1 10.13 usec
PLW1 51.00000000 W

===== CHANNEL f2 =====
SF02 400.1316005 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 11.50800037 W
PLW12 0.31077999 W

F2 - Processing parameters
SI 262144
SF 100.6127690 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40
SR 0 Hz

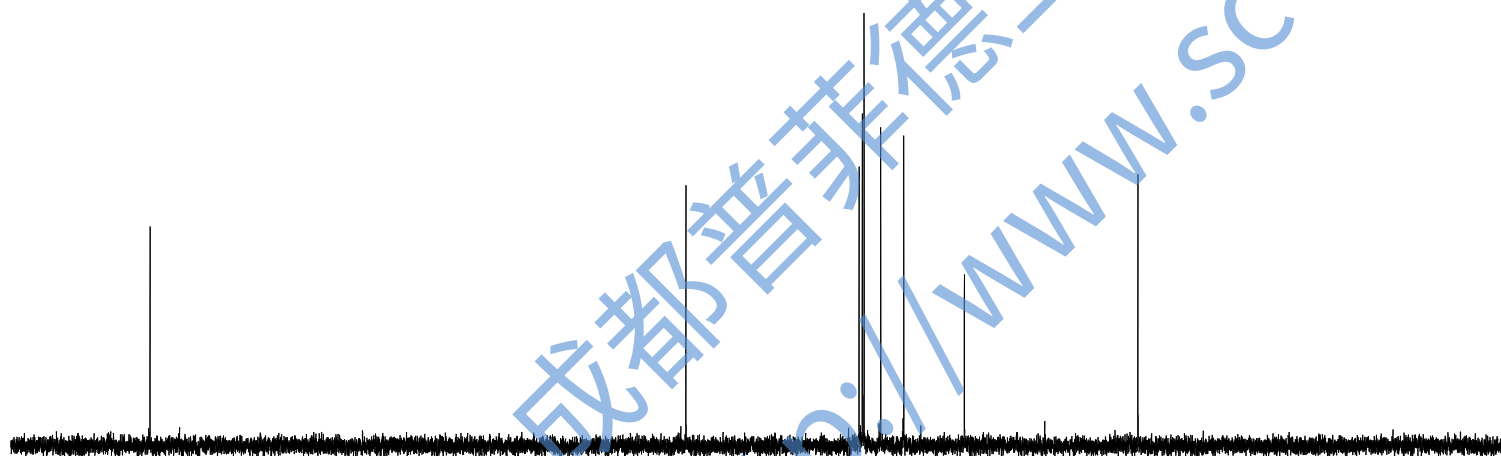



Current Data Parameters
NAME JXLG-13C NMR D20
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20161019
Time 10.16
INSTRUM spect
PROBHD 5 mm PABBO BB/
PULPROG zgig30
TD 65536
SOLVENT D2O
NS 366
DS 4
SWH 24038.461 Hz
FIDRES 0.366798 Hz
AQ 1.3631488 sec
RG 202.5
DW 20.800 usec
DE 6.50 usec
TE 301.2 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1

===== CHANNEL f1 =====
SF01 100.6228298 MHz
NUC1 13C
P1 10.13 usec
PLW1 51.00000000 W

===== CHANNEL f2 =====
SF02 400.1316005 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 11.50800037 W
PLW12 0.31077999 W

F2 - Processing parameters
SI 262144
SF 100.6127690 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40
SR 0 Hz

