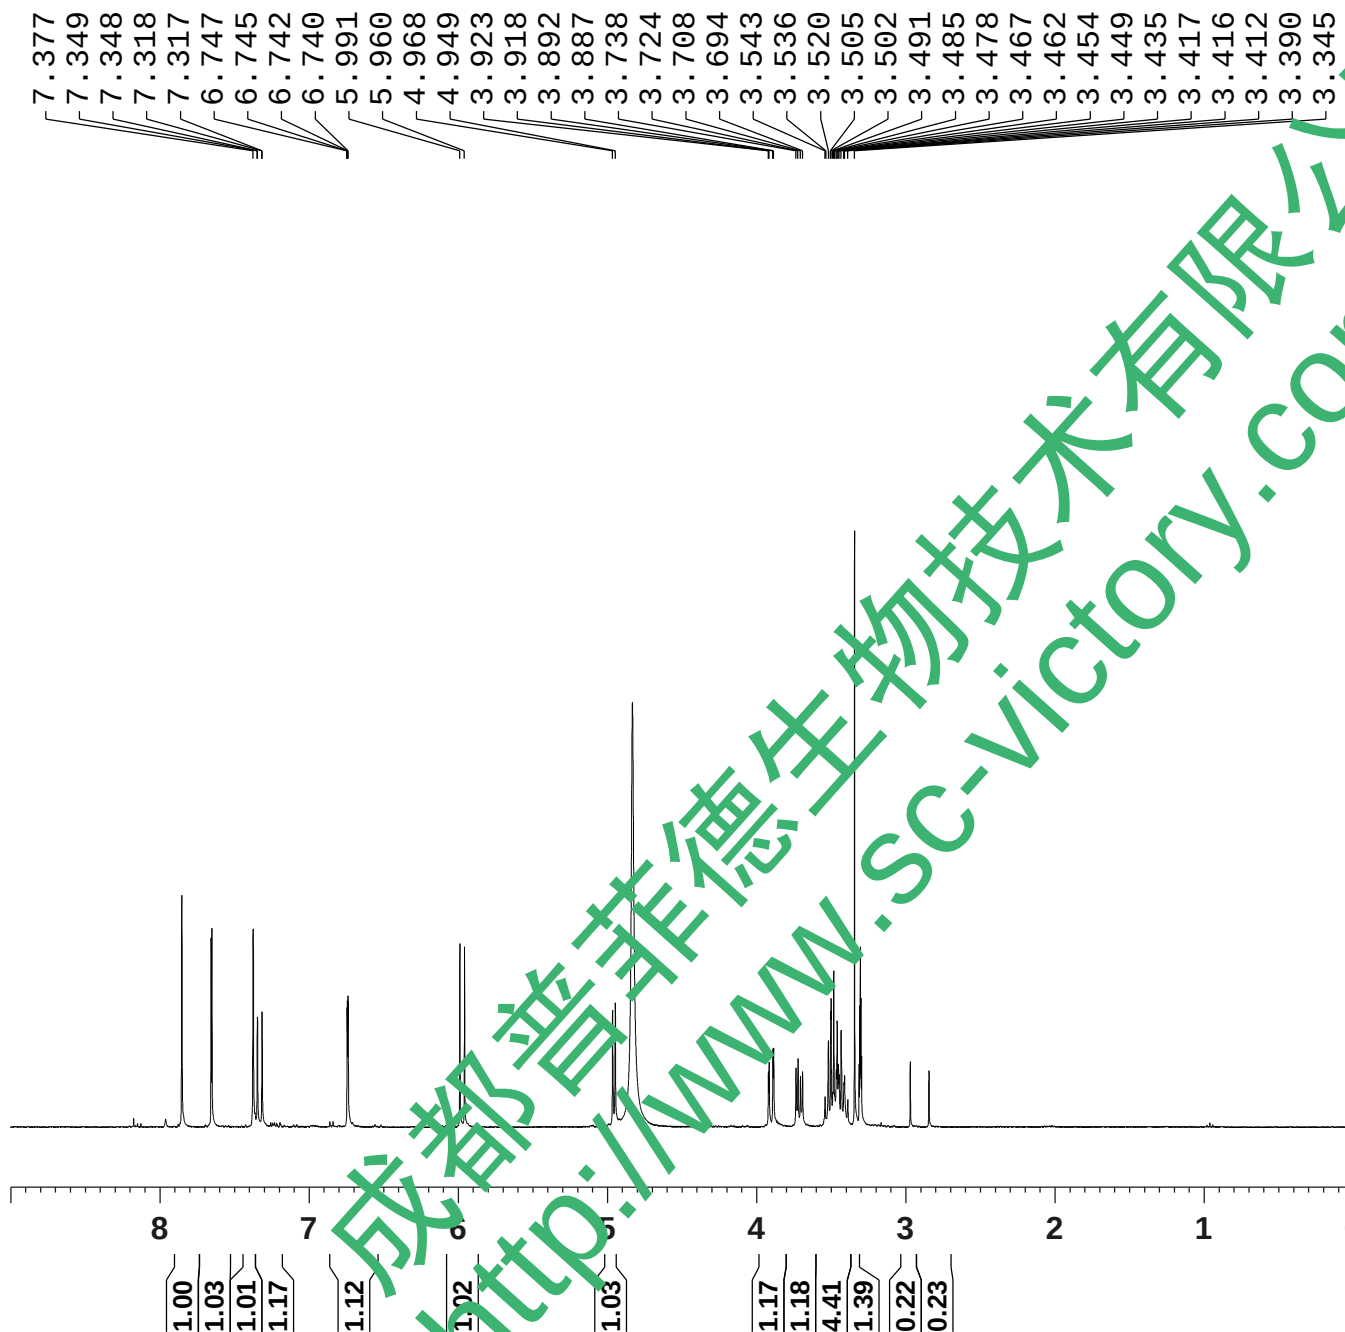


Current Data Parameters
NAME BGZ 1#-1H NMR CD3OD
EXPNO 5
PROCNO 1


F2 - Acquisition Parameters

INSTRUM spect
PROBHD 5 mm PABBO BB/
PULPROG zg30
TD 65536
SOLVENT MeOD
NS 4
DS 2
SWH 8012.820 Hz
FIDRES 0.122266 Hz
AQ 4.0894465 sec
RG 81.22
DW 62.400 usec
DE 6.50 usec
TE 301.2 K
D1 1.00000000 sec
TD0 1

===== CHANNEL f1 =====
SF01 400.1324710 MHz
NUC1 1H
P1 14.79 usec
PLW1 11.50800037 W

F2 - Processing parameters
SI 65536
SF 400.1300091 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00
SR 9.13 Hz

—171.46
—157.18
—154.93
—146.50
—138.79
—123.47
—123.09
—123.07
—121.34
—107.47
—103.28
—100.00
—78.19
—78.08
—74.91
—71.31
—62.49

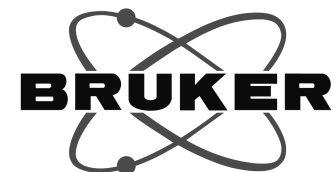

Current Data Parameters
NAME BGZ 1#-13C NMR CD3OD
EXPNO 6
PROCNO 1

F2 - Acquisition Parameters

INSTRUM spect
PROBHD 5 mm PABBO BB/
PULPROG zgig30
TD 65536
SOLVENT MeOD
NS 545
DS 4
SWH 24038.461 Hz
FIDRES 0.366798 Hz
AQ 1.3631488 sec
RG 202.5
DW 20.800 usec
DE 6.50 usec
TE 301.3 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1

===== CHANNEL f1 =====
SF01 100.6228298 MHz
NUC1 13C
P1 10.13 usec
PLW1 51.00000000 W

===== CHANNEL f2 =====
SF02 400.1316005 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 11.50800037 W
PLW12 0.31077999 W

F2 - Processing parameters
SI 262144
SF 100.6126317 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40
SR -137.28 Hz

